
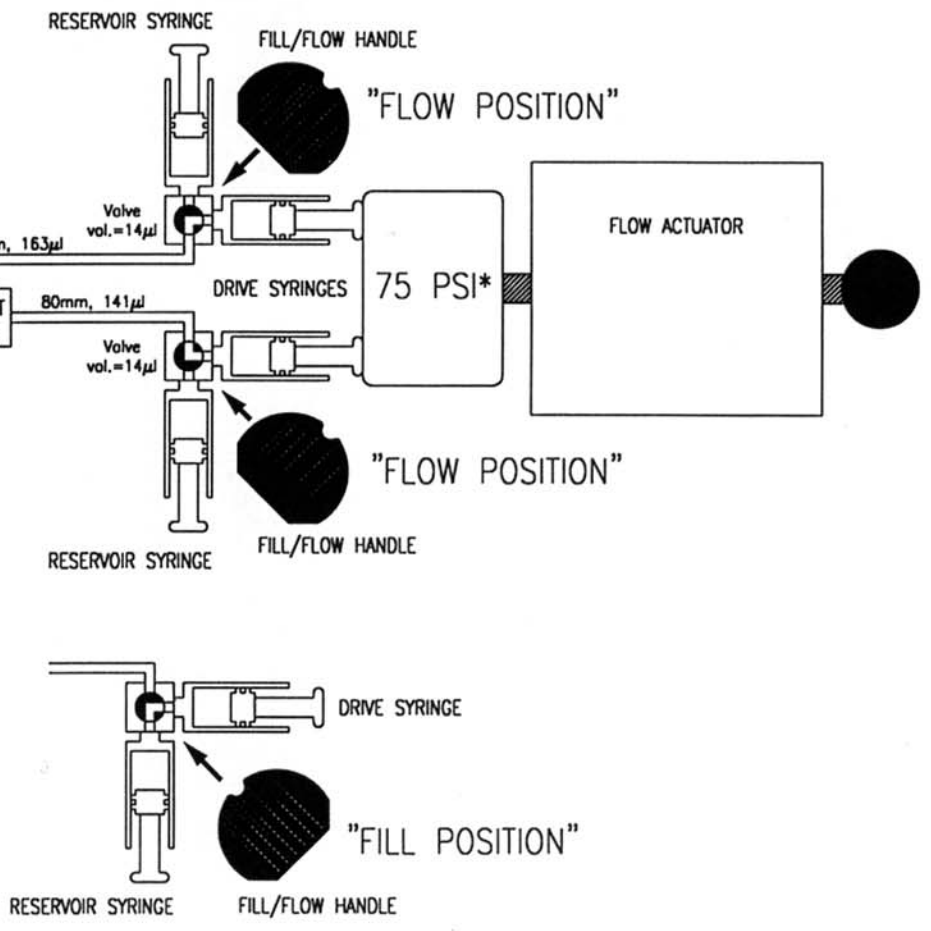
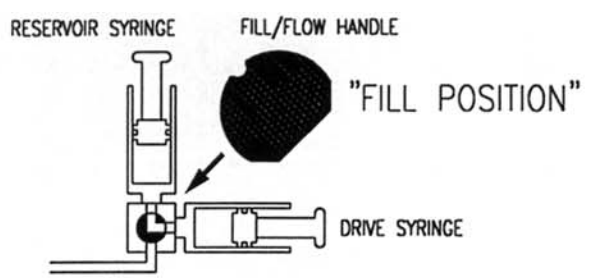
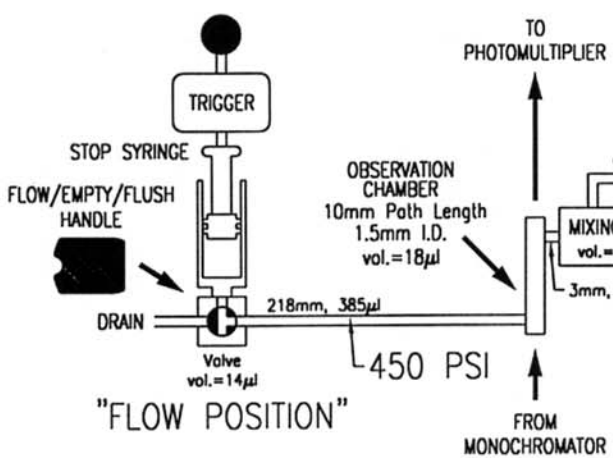


BLOCK DIAGRAM OF OLIS U.S.A. STOPPED-FLOW With Low-Temp 10mm Flow Cell

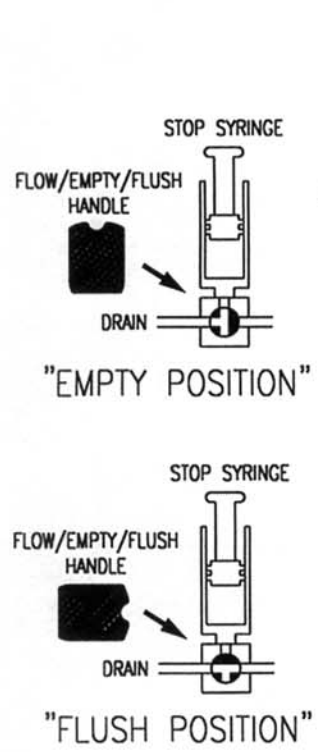

VOLUMES

378 μl from Drive Syringe to filled Observation Chamber
777 μl from Drive Syringe to Stop Syringe

* Exceeding 75 PSI at the drive syringe will void your warranty; 65 PSI is recommended every 5 lb. at the drive syringe increases the pressure at the stop syringe by 50 lb.